



miR-ID[®]: miRNA quantification assays

Experimental Protocol

support@somagenics.com
www.somagenics.com

Table of Contents

I.	Overview	5
II.	miR-ID [®] Kit Contents	6
III.	User Supplied Reagents and Laboratory Equipment (not included)	6
IV.	Experimental Protocol	7
V.	Appendix A: Overview of Working Steps for Singleplex Reactions	12
VI.	Appendix B: Overview of Working Steps for Multiplex Reactions	13

For Research Use Only.

Information in this document is subject to change without notice.

SOMAGENICS DISCLAIMS ALL WARRANTIES WITH RESPECT TO THIS DOCUMENT EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO THOSE OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE, TO THE FULLEST EXTENT ALLOWED BY LAW, IN NO EVENT SHALL SOMAGENICS BE LIABLE, WHETHER IN CONTRACT, TORT, WARRANTY, OR UNDER ANY STATUTE OR ON ANY OTHER BASIS FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING BUT NOT LIMITED TO THE USE THEREOF, WHETHER OR NOT FORESEEABLE AND WHETHER OR NOT SOMAGENICS IS ADVISED OF THE POSSIBILITY OF SUCH DAMAGES.

NOTICES TO PURCHASER:

LIMITED LICENSE

The purchase of this product conveys to the purchaser the limited, non-transferable right to use the purchased amount of the product only to perform internal research for the sole benefit of the purchaser. No right to resell this product or any of its components is conveyed expressly, by implication, or by estoppel. This product is for internal research purposes only and may not be transferred to third parties, resold, modified for resale, or used to manufacture commercial products or to provide a service to third parties without prior written approval of SomaGenics, Inc. For information on obtaining additional rights, please contact: bd@somagenics.com.

miR-ID[®]/miR-Direct[®] CUSTOMER USE AGREEMENT

When purchasing products incorporating SOMAGENICS' miR-ID[®] and miR-Direct[®] technologies you agree to the following terms and conditions. These terms and conditions constitute the use agreement ("Use Agreement") for products and materials containing miR-ID[®] and miR-Direct[®] sample preparation products, primer designs, primer sequences, primers, probe designs, probes and/or assays (together "miR-ID[®] and miR-Direct[®] Materials"). This Use Agreement creates a binding contract between you and SOMAGENICS for the purchase and use of our miR-ID[®] and miR-Direct[®] Materials.

Under this Use Agreement, SOMAGENICS retains all right, title and interest in and to the miR-ID[®] and miR-Direct[®] Materials. All custom services derived from miR-ID[®] and miR-Direct[®] Materials are provided on a non-exclusive basis (see www.somagenics.com; Terms and Conditions for Custom Services). miR-ID[®] and miR-Direct[®] Materials are provided for Research Use Only and no other rights are conveyed by this Use Agreement. You are expressly prohibited from independently recreating miR-ID[®] and miR-Direct[®] Materials which are proprietary to SOMAGENICS. If you require additional rights please contact: bd@somagenics.com.

This product is covered by issued and pending patents.

TRADEMARKS

miR-ID[®] and miR-Direct[®] are the Registered Trademarks of SomaGenics, Inc. All other brands and names contained herein are the property of their respective owners.

support@somagenics.com


www.somagenics.com

miR-ID[®]: miRNA Detection Assays

I. Overview

miR-ID[®] is a novel platform for detecting miRNA using a circularization-based RT-qPCR method. miR-ID[®] is highly sensitive, uses single-dye detection, and can discriminate miRNA isoforms with single nucleotide differences at any position along the molecule. The miR-ID[®] assay is designed to detect specific miRNAs in biological samples and works well with all sample sources, including total RNA. miR-ID[®] is capable of detecting 2'-OMe modifications on the 3' ends of piRNAs in animals and all small RNAs in plants.

The assay consists of a 3-step protocol in which Steps 1 and 2 (see flowchart below) can be performed in multiplex. If working with synthetic miRNAs, these RNAs must have 5'-p and 3'-OH groups at their termini.

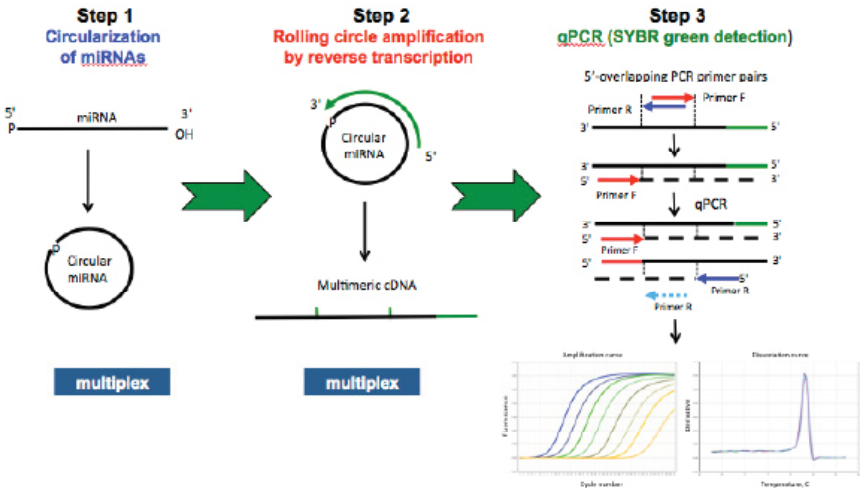

Schematic of miR-ID[®]. **Step 1:** Circularization of linear miRNAs; **Step 2:** Reverse transcription mediated by rolling circle amplification to obtain multimeric cDNA; **Step 3:** Quantification of the amplicon by RT-qPCR using highly sequence-specific 5'-overlapping primers and SYBR Green detection. Kumar et al (2011) *RNA* 17:365.

II. miR-ID[®] Kit Contents

Store all components at -20°C

1. Circularization Reaction Mix
2. RT Primer/s
3. RT Reaction Mix
4. RT Dilution Buffer
5. Nuclease-free Water
6. PCR Primers

III. User-supplied Reagents, Consumables, and Laboratory Equipment (not included)

Reagents

- CircLigase II (Lucigen / LGC, cat# CL9021K)
- RNaseOUT (Thermo Fisher Scientific, cat# 10777019)
- Superscript IV Reverse Transcriptase (Thermo Fisher Scientific, cat# 18090010)

SYBR green reagents such as

- 2X iQ SYBR Green Supermix (BioRad, cat# 170-8880)
- Rox reference dye (Thermo Fisher Scientific, cat# 12223012)

Consumables

- Pipettes and nuclease-free filtered pipette tips for volumes 2 to 100 µl.
- RNase-free microfuge tubes (1.5 ml).
- PCR tubes or PCR strip tubes.
- Micro-Amp Fast Optical 96-Well Reaction Plate, for example Thermo Fisher Scientific cat# 4346906
- Micro-Amp Clear Adhesive Film, for example Thermo Fisher Scientific cat# 4360954

Equipment

- Ice bucket/freezer plate for reagents and enzymes
- Centrifuge for 96-well plates
- Thermal Cycler
- Real-time qPCR instrument, for example 7500-Real Time PCR System (Thermo Fisher Scientific)

support@somagenics.com
www.somagenics.com

IV. Experimental Protocol

Subsection A: singleplex (yields 20 μL cDNA)

1. miRNA circularization

- 1.1. Allow Circularization buffer and RNA samples to thaw on ice.
- 1.2. For each biological sample combine components listed below. When assaying multiple samples, make a combined mastermix and allow 10% overage for pipetting loss. Gently mix components and pulse-spin to collect liquid on bottom. Keep on ice. Aliquot 5 μL into each PCR tube (single or strip tubes).

Reagent	Volume
Circularization Reaction Mix	2.5 μL
RNA (1 to 20 ng total)	2.0 μL
RNaseOUT	0.3 μL
Circ Ligase II	0.2 μL
Total	5.0 μL

- 1.3. Incubate the circularization mixture at 60°C for 15 minutes and transfer to ice.

2. Reverse transcription

- 2.1. Allow RT buffer and RT primer(s) to thaw on ice.
- 2.2. In an RNase-free tube, combine components listed in the table below. When assaying multiple samples, make a combined mastermix and allow 10% overage for pipetting loss. Gently mix components and pulse-spin to collect liquid on bottom. Keep on ice.

Reagent	Volume
RT Reaction Mix	6.4 μL
RT Primer/s	0.2 μL^*
SuperScript IV Enzyme	0.4 μL
Nuclease-free Water	8.0 μL^*
Total	15.0 μL

* (If only one sample is prepared, the RT primer should be diluted 10 times with RT dilution buffer. 2 μL of the diluted RT primer will be added and the volume of the nuclease-free water will be reduced to 6.2 μL)

- 2.3. Aliquot 15 μL of the mix into each sample, yielding a final volume of 20 μL . Gently mix components and pulse-spin to collect liquid on bottom.
- 2.4. Place tubes into thermal cycler and run the following parameter values:

Temperature	Time
42°C	60 min
80°C	10 min
4°C	∞

- 2.5. Mix gently and centrifuge briefly.

***Stopping point*:** RT reactions may be used directly in qPCR or stored at -20°C.

Subsection B: multiplex (yields 80 μL cDNA)

1. miRNA circularization

- 1.1. Allow Circularization buffer and RNA samples to thaw on ice.
- 1.2. For each biological sample combine components listed below. When assaying multiple samples, make a combined mastermix and allow 10% overage for pipetting loss. Gently mix components and pulse-spin to collect liquid on bottom. Keep on ice. Aliquot 20 μL into each PCR tube (single or strip tubes).

Reagent	Volume
Circularization Reaction Mix	10.0 μL
RNA (1 to 20 ng total)	8.0 μL
RNAseOUT	1.2 μL
Circ Ligase II	0.8 μL
Total	20.0 μL

- 1.3. Incubate the circularization mixture at 60°C for 15 minutes and transfer to ice.

2. Reverse transcription (multiplex)

- 2.1. Allow the RT buffer and RT primers to thaw on ice.
- 2.2. Prepare the RT primer mix using the supplied RT primers: for each biological sample that will be analyzed, pipet 0.8 μl of each primer into an RNase-free tube and add nuclease-free water to a final volume of 32.8 μl (or multiples thereof if multiple biological samples are being analyzed).
- 2.2. In an RNase-free tube, combine the components listed in the table below. When assaying multiple samples, make a combined mastermix and allow 10% overage for pipetting loss. Gently mix components and pulse-spin to collect liquid on bottom. Keep on ice.

Reagent	Volume
RT Reaction Mix	25.6 μl
RT Primer Mix	32.8 μl
SuperScript IV Enzyme	1.6 μl
Total	60.0 μl

- 2.3. Aliquot 60 μl of the mix into each sample, yielding a final volume of 80 μl . Gently mix components and pulse-spin to collect liquid on bottom.
- 2.4. Place tubes into thermal cycler and run the following parameter values:

Temperature	Time
42°C	60 min
80°C	10 min
4°C	∞

- 2.5. Mix gently and centrifuge briefly.

***Stopping point*:** RT reactions maybe be used directly in qPCR or stored at -20°C.

3. Quantitative RT-PCR

The qPCR step is always performed in singleplex (each miRNA is assayed in a single reaction), even if circularization and RT are performed in multiplex. Forward and reverse primers for each miRNA are included in the miR-ID kit. A typical 20 μ l reaction for a single miRNA is described below. Note that each RT reaction of the multiplex setup serves as template for qPCR for each miRNA assay.

NOTE: Refer to the vendor's user guide for instructions on setting up the qPCR master mix. The following master mix preparation is specific for BioRad's 2x iQ SYBR Green Supermix.

- 3.1. Allow the 2x qPCR master mix (light sensitive), Rox reference dye, qPCR primers, and RT reactions to thaw on ice.
- 3.2. A separate master mix needs to be prepared for each assayed miRNA. Calculate master mix components for each miRNA by multiplying the reagent volume by the number of samples and by the number of technical repeats (triplicate analysis is recommended). Allow 10% overage for pipetting loss. Mix gently and spin down the qPCR master mix.

Reagent	Volume
2x iQ SYBR Green Supermix	10.0 μ l
Nuclease-free Water	7.1 μ l
qPCR Primers (miRNA specific)	0.6 μ l
Rox Reference Dye	0.3 μ l
Total	18.0 μl

- 3.3. Pipet 18 μ l of the appropriate master mix into wells of a qPCR plate.
- 3.4. Pipet 2 μ l cDNA from the RT reaction into the appropriate individual wells.
- 3.5. Seal qPCR plate with optical seal and centrifuge to bring the solution to the bottom of the plate.

- 3.6. Set up the following program for the real-time thermal cycler and start the run.

Assay: Standard Curve (Absolute Quantification)

Run mode: Standard 7500

Step Type	Temperature	Time
HOLD	50°C	2 min
HOLD	95°C	3 min
CYCLE (40 cycles)	95°C	15 sec
	56°C	45 sec
	66°C + 0.1 per cycle	30 sec
	67°C + 0.2 per cycle*	30 sec
Include standard melting curve profile at the end of 40 cycles		


* Set up data collection at this step.

Data Analysis


For instructions on how to analyze and export raw Ct values, refer to the appropriate instrument user guide. The general process typically involves the following procedures:

- View the amplification plots.
- Set the baseline and threshold values and obtain Ct values.
- Analyze melting curves for PCR products.

V. Appendix A: Overview of Working Steps for Singleplex Reactions

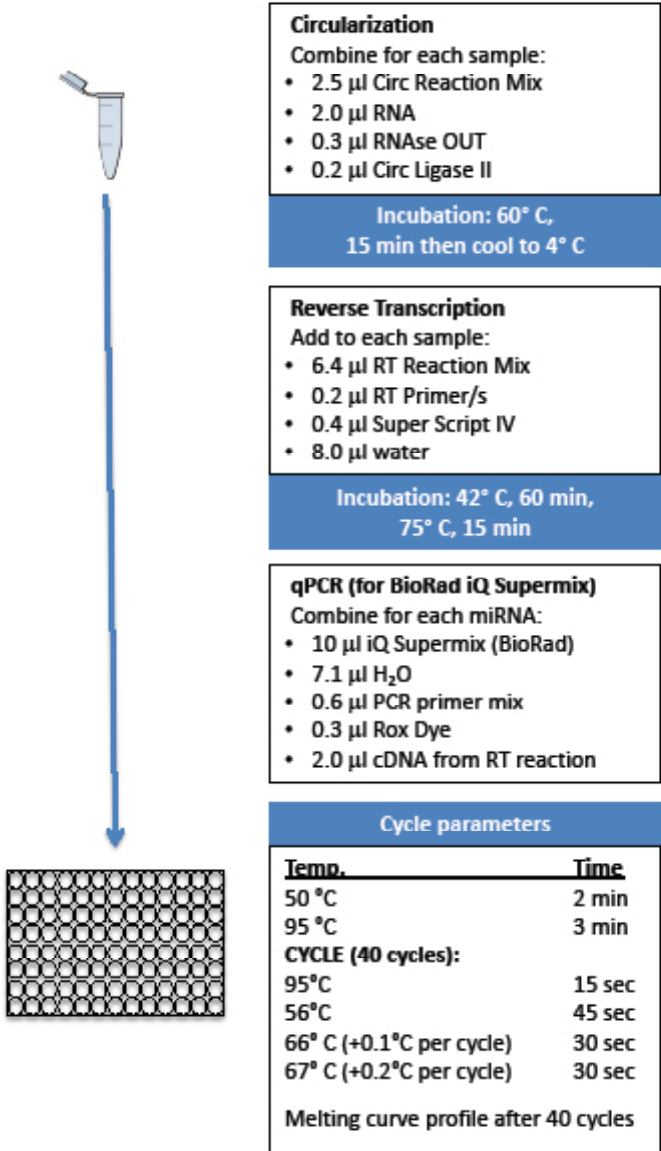

VI. Appendix B: Overview of Working Steps for Multiplex Reactions

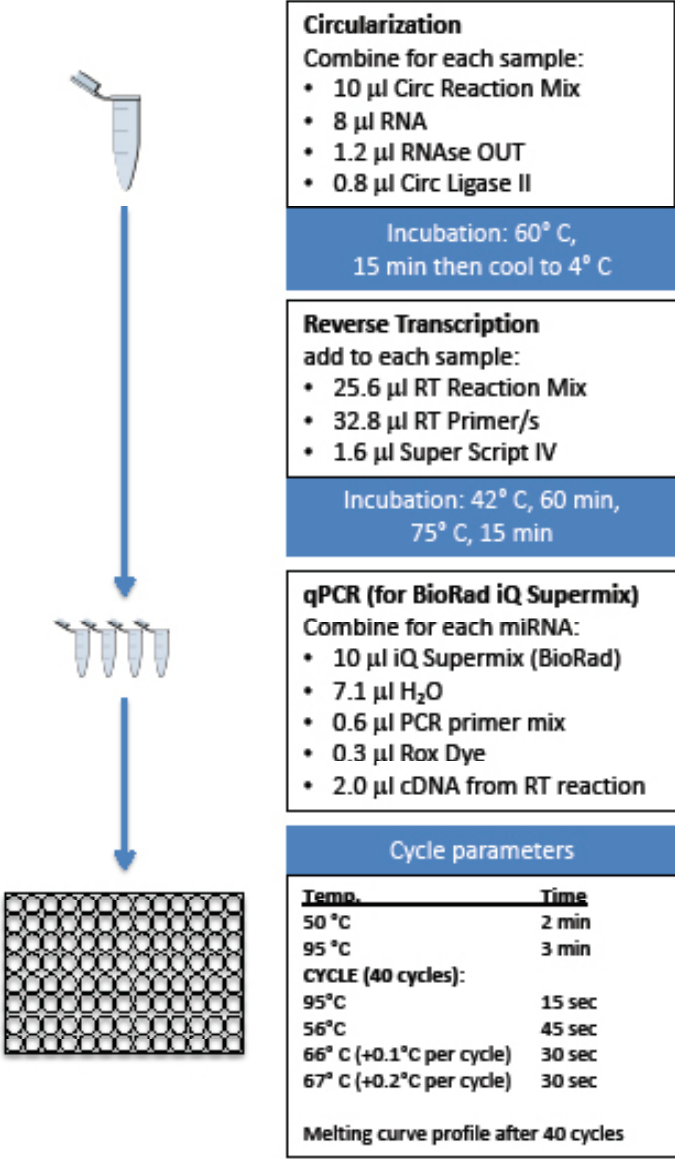

support@somagenics.com
www.somagenics.com

support@somagenics.com
www.somagenics.com